

RESEARCH

Open Access



Antifungal activity, mechanical properties, and accuracy of three-dimensionally printed denture base with microencapsulated phytochemicals on varying post-polymerization time

Ye-Hyeon Jo^{1†}, Won-Jun Lee^{2†}, Ji-Hyun Lee¹ and Hyung-In Yoon^{2*}

Abstract

Background: Studies on the antifungal activity, flexural strength, Vickers hardness, and intaglio surface trueness of three-dimensionally printed (3DP) denture bases with microencapsulated phytochemicals with respect to changes in post-polymerization time (PPT) are lacking.

Methods: Specimens of various shapes and dimensions were fabricated with a 3DP denture base resin mixed with 5 wt% phytoncide-filled microcapsules. Each specimen was subjected to different PPT protocols of 5, 10, 20, and 30 min. Specimens without microcapsules with 5-min PPT were used as the negative control group. Cell colonies were counted to evaluate antifungal activity. Three-point bending and Vickers hardness tests were performed to measure the flexural strengths and hardness of the specimens. Fourier-transform infrared spectrometry was used to inspect the degree of conversion (DC). The intaglio surface trueness was measured using root-mean-square estimates calculated by superimposition analysis. A non-parametric Kruskal–Wallis test or one-way analysis of variance was performed ($\alpha = 0.05$).

Results: The specimens with microcapsules and 10-min PPT showed the highest antifungal activity among the tested groups. Compared with the positive control group (5-min PPT), the specimens with PPTs of 10 min or longer showed significantly higher mean flexural strength, higher DC, greater hardness, and better trueness (all, $P < 0.05$). Except for the difference in antifungal activity, no statistically significant differences were detected between the specimens subjected to 10-, 20-, and 30-min PPT.

Conclusion: The 3DP denture base filled with microencapsulated phytoncide showed different antifungal activity and physical properties on changing PPT. The 3DP denture base containing phytoncide-filled microcapsules at 5 wt%

[†]Ye-Hyeon Jo and Won-Jun Lee contributed equally to this work as first authors.

*Correspondence: drhiy226@snu.ac.kr

² Department of Prosthodontics, School of Dentistry and Dental Research Institute, Seoul National University, 101, Daehak-ro, Jongno-gu, Seoul 03080, Republic of Korea

Full list of author information is available at the end of the article



© The Author(s) 2022. **Open Access** This article is licensed under a Creative Commons Attribution 4.0 International License, which permits use, sharing, adaptation, distribution and reproduction in any medium or format, as long as you give appropriate credit to the original author(s) and the source, provide a link to the Creative Commons licence, and indicate if changes were made. The images or other third party material in this article are included in the article's Creative Commons licence, unless indicated otherwise in a credit line to the material. If material is not included in the article's Creative Commons licence and your intended use is not permitted by statutory regulation or exceeds the permitted use, you will need to obtain permission directly from the copyright holder. To view a copy of this licence, visit <http://creativecommons.org/licenses/by/4.0/>. The Creative Commons Public Domain Dedication waiver (<http://creativecommons.org/publicdomain/zero/1.0/>) applies to the data made available in this article, unless otherwise stated in a credit line to the data.

concentration and subjected to 10-min PPT exhibited sufficient antifungal activity as well as mechanical properties and accuracy within clinical acceptance.

Keywords: 3D printing, Denture base, Phytoncide, Microcapsule, Antifungal activity, Post-polymerization time

Introduction

Polymethyl methacrylate (PMMA) resin has been used in the fabrication of removable denture prostheses for a long time [1–3]. It has several advantages, such as favorable esthetics, biocompatibility, low cost, and simple processing [1, 4]. However, fracture of the acrylic resin is frequently reported in 57–64% of all cases of clinical failures of removable denture prostheses [5, 6]. Furthermore, the conventional pack and press technique of denture fabrication has been reported to be susceptible to dimensional change owing to polymerization shrinkage [7, 8]. With the progress of computer-aided design and computer-aided manufacturing (CAD-CAM) technology, additive manufacturing methods, also known as three-dimensional (3D) printing, have been applied to the workflow of fabricating denture prostheses [9, 10]. 3D-printed (3DP) denture bases can be manufactured with unlimited shape reproduction, sufficient precision, and physical properties using a photo-polymerizable acrylic resin [9, 10], which simplifies the workflow of removable dentures [10]. Recently, the clinical applicability of 3DP denture bases has been substantiated by several researchers. Denture bases for edentulous arches fabricated using digital light processing (DLP) showed favorable tissue surface adaptation and dimensional accuracy, which was similar to or better than that of bases manufactured by 5-axis milling [11, 12]. A clinical study by Yoon et al. revealed that denture bases produced via 3D printing were more advantageous than those produced via milling in terms of tissue surface adaptation due to better reproduction of the complex contour of the edentulous ridge [13]. Furthermore, the adaptation of the denture base to the tissue surface can be improved by optimizing the build angle during the DLP-based workflow [14]. However, regardless of the manufacturing workflow, the acrylic resin material used for denture bases has an inherent drawback, as the intaglio surface could be a potential reservoir of oral microorganisms, such as bacteria or fungi, due to surface roughness, geometric irregularities, and porosity [15–17].

Denture stomatitis is an inflammatory fungal infection that affects approximately 50–75% of otherwise healthy denture wearers and is the most common form of oral candidiasis [18–20]. Apart from antifungal treatment, conditioning of the abused tissue, cleansing of the affected mucosa or denture surface, and fabrication of new dentures are the treatment of choice. Due to

concerns regarding systemic adverse reactions caused by oral antifungal drugs [21, 22], alternative approaches, such as photodynamic treatment [23] or adjunct physical cleansing, have been recently used to effectively treat denture stomatitis [24]. In addition, imparting antibacterial activity to the denture material by directly coating or adding antibacterial compounds has also been proposed [25–28]. In particular, a novel additive manufacturing technique to directly add substances with antibacterial properties to the denture material has been suggested. The substances selected for this purpose were certain oxides or chemical compounds and phytochemicals, which are naturally derived substances with antimicrobial activities [29–31]. The antifungal properties of phytochemicals, such as phytoncide oil, have been previously reported [32, 33]. The phytoncide could reduce optical density and viability of fungal cells as well as increase the number of morphologically atypical cells [34]. Recent studies reported the development of a denture base with antifungal properties by incorporating phytoncide into PMMA resin [35, 36]. Furthermore, microencapsulation of phytoncide oil extract was recommended to achieve continuous effect of its antimicrobial activity [30, 36].

A novel method using microencapsulation and additive manufacturing has been recently introduced to incorporate the antifungal activity of phytoncide extract into the acrylic resin for 3DP denture bases and maintain its effectiveness for a certain period without compromise [31]. 3DP denture bases with phytoncide-filled microcapsules at concentrations ranging from 6 to 8 wt% showed sufficient antifungal effects on fungal cell colonies [31]. However, they showed mediocre mechanical properties (flexural strength or hardness), which were barely comparable with those of bases without microcapsules, and exhibited lesser dimensional accuracy, which was clinically acceptable [37]. Since denture bases should withstand masticatory forces, resist surface wear, and guarantee intimate tissue surface adaptation, the physical properties and dimensional accuracy of the 3DP denture base with phytoncide-filled microcapsules must be improved further. Among the various parameters used for 3D printing, the light exposure time during the post-polymerization has been reported to affect the accuracy and strength of 3DP resin materials [38–40]. The dimensional accuracy (trueness and precision), degree of conversion, and mechanical properties (flexural strength and Vickers hardness) of resin-based 3DP objects have been

significantly improved by changing the post-polymerization time (PPT) [38–40].

To the best of our knowledge, there has been no research on the effect of PPT on the antifungal activity, physical properties, and accuracy of 3DP denture base resins containing phytochemical-filled microcapsules. Therefore, this in-vitro study aimed to evaluate 3DP denture bases with microencapsulated phytochemical (phytoncide oil extract) in terms of antifungal activity, flexural strength, Vickers hardness, and intaglio surface trueness with respect to changes in PPT (5, 10, 20, and 30 min). The null hypothesis was that the antifungal activity, flexural strength, Vickers hardness, and intaglio surface trueness of 3DP denture bases filled with microencapsulated phytoncide would not be affected by the changes in PPT.

Methods

A disc-shaped specimen with a diameter of 15 mm and thickness of 5 mm was virtually designed with universal CAD software (TinkerCAD, Autodesk, Quebec) to test the antifungal activity, Vickers hardness, and degree of conversion. A bar-shaped specimen ($65 \times 10 \times 3.3 \pm 0.2$ mm) was designed to measure the flexural strength of the printed denture base materials in accordance with ISO 20975-1:2013 [41]. A maxillary denture base-shaped specimen was designed to evaluate the trueness of the intaglio surface after 3D printing. An edentulous maxillary dentiform with soft gingiva (EDE1001-UL-UP-DPM, Nissin, Japan) was digitized to obtain maxillary full-arch scan data (i500; Medit, Korea). A maxillary complete denture base (reduced to 50% of its size) was virtually designed using dental CAD software (3Shape Dental Designer; 3Shape, Denmark) and saved in a standard tessellation language (.stl) format as reference CAD data.

A 3D-printable resin (NextDent Denture 3D+, Vertex Dental BV, Soesterberg, Netherlands), designed for the fabrication of removable denture bases, was used in this study. Phytoncide oil was extracted from *Pinus densiflora* (Cleandiox. Ltd., Korea) and microencapsulated to prepare functional microcapsules with antifungal activity [31]. Detailed process of microencapsulation was previously reported in the study by Jeon et al. [31]. Briefly, the phytoncide oil and the styrene-maleic anhydride copolymer solution was mixed to form droplets. Melamine/urea/formaldehyde was then dissolved in the mixture to form a wall of the microcapsule. After aging for cohesion, the microcapsules were sieved and dried. The phytoncide-filled microcapsules were carefully mixed with the 3D-printable denture base resin at a concentration of 5 wt% [31, 37]. A dispersant (DISPERBYK-111, BYK, Germany) was added at 20 wt% of the mass (g) of the phytoncide-filled microcapsules to the mixture for uniform

dispersion. All 3DP denture base resin specimens with various shapes and dimensions were produced using the microcapsule-resin mixture and a DLP-based 3D printer (MAX UV, ASIGA, Australia) with a wavelength of 385 nm. The layer thickness and build orientation for each 3D printing were set to 50 μ m and 0°, respectively, and horizontally positioned to build the platform (Asiga Composer 1.2.12, Asiga, Australia). Specimens of 3DP denture base resin with no microcapsules and dispersant agent were also manufactured according to the abovementioned protocols and parameters as the control group. All specimens were cleaned using ethanol in a washing machine as per the manufacturer's instructions (Form wash, Formlabs, Somerville, USA) for 10 min. The support structures were carefully removed, and no further adjustments were made to the specimen surfaces.

After cleansing and removing the support structure, the disc-shaped 3DP denture resin specimens (Fig. 1) underwent post-polymerization with a curing unit (Cure M U102H, Graphy, Seoul, Korea). The 5-min PPT, a default protocol recommended by the manufacturer, was applied to the 3DP denture resin discs with phytoncide-filled microcapsules for the control group (positive control). For the experimental groups, 3DP denture resin discs with microcapsules subjected to three different PPTs (10-, 20-, and 30-min) were evaluated. As a negative control, the 3DP denture resin discs without microcapsules subjected to 5-min PPT (default protocol) were also tested. After post-processing as recommended by the manufacturers, the as-printed surface of each 3DP denture resin specimen, opposing the attached area of the support structures, was used as a testing surface for further analysis.

Candida albicans (ATCC 10,231, *C. albicans*), provided by the Korean Collection for Oral Microorganisms, was cultured in Sabouraud dextrose (SD) broth at 37 °C and used to assess the antifungal activity of the 3DP denture resin discs with phytoncide-filled microcapsules. The 3DP discs with and without microcapsules ($n=5$ each), subjected to different PPT protocols, were placed at the bottom of a 12-well plate. To each well, 2 mL of *C. albicans* suspension (optical density: 0.02, equivalent to 2×10^4 microbial cells per mL) was added and incubated for 24 h at 37 °C. The discs were rinsed with Dulbecco's phosphate-buffered saline (DPBS) and transferred to tubes filled with 5 mL of SD broth. Each disc was ultrasonicated at 40 kHz for 5 min to detach the microbial cells from its surface (NXPC-B5020SB, Kodo, Korea) [42]. The absorbance value of the fungal solution (200 μ L) was measured using a microplate reader (Epoch2, BioTek, USA) at a wavelength of 600 nm. Subsequently, 10 μ L of the diluted fungal solution was seeded onto an SD agar plate and incubated for 24 h at

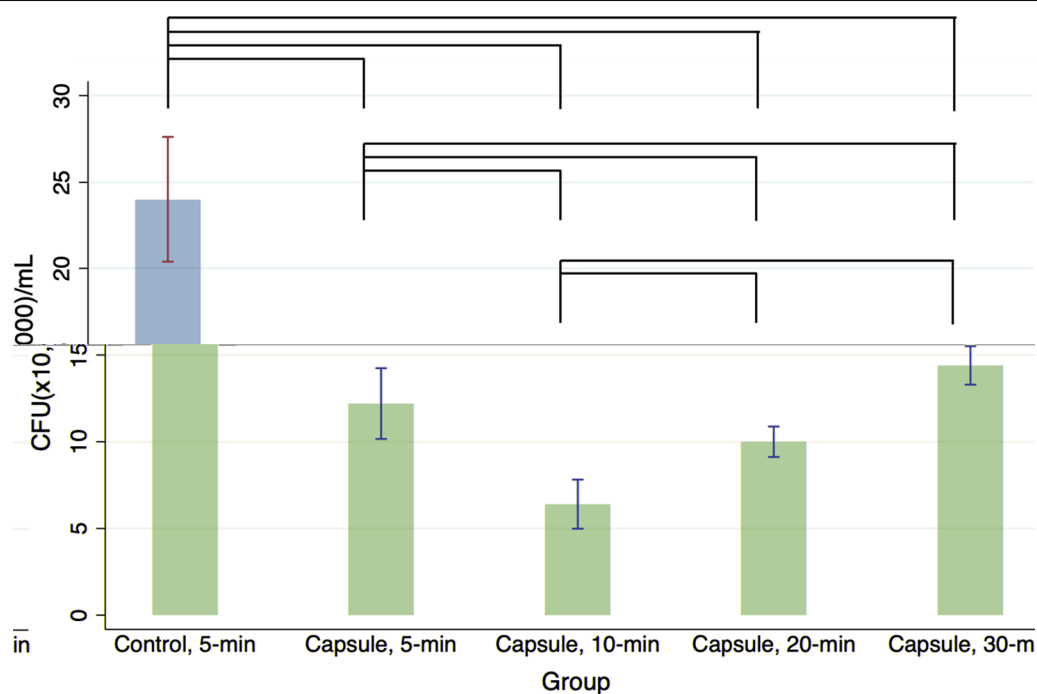


Fig. 1 Colony-forming units per milliliter (CFU/mL) of *Candida albicans* detached from 3D-printed denture base resin discs and subjected to different post-polymerization time (PPT) protocols: 5-min, 10-min, 20-min, and 30-min. Control: 3D-printed denture base resin discs without microcapsules; Capsule: 3D-printed denture base resin discs with 5 wt% phytoncide-filled microcapsules. Significant differences between the groups are marked with black lines ($P < 0.05$)

37 °C. For the SEM analysis, the discs were cleaned with DPBS and fixed in 2.5% (v/v) glutaraldehyde (Sigma-Aldrich, USA) for 2 h. The fixative was aspirated and cleaned with DPBS and post-fixed in 1% osmium tetroxide for 30 min. After fixation, samples were dehydrated in a graded series of ethanol solutions. After critical point drying, the specimens were sputter-coated with Pt and microscopically examined using field-emission scanning electron microscopy (FE-SEM, Apreo S, Thermo Fisher Scientific, MA, USA) at 10 kV. The colonies were counted as colony-forming units per milliliter (CFU/mL), and the morphological changes in the fungal cell colonies on the specimen surfaces were examined.

To measure the flexural strength of the denture base materials in accordance with ISO 20795-1:2013 [41], the bar-shaped 3DP denture resin specimens ($n=10$) subjected to different PPTs with and without microcapsules were prepared and stored in 37 °C distilled water for 50 h. The flexural strength of each bar-shaped specimen was measured using a three-point bending test apparatus with a universal testing machine (Instron 8871; Instron, Canton, MA, USA) of 5kN load cell at a crosshead speed of 5 mm/min. The flexural strength (FS) was computed using the following equation:

$$FS = \frac{3Pl}{2bd^2},$$

where P is the maximum load before fracture, l is the distance between the supports (50 mm), b is the specimen width, and d is the specimen thickness. After testing, the fractured surfaces were sputter-coated with Pt (5-nm layer thickness) and observed using FE-SEM for fractographic analysis.

A Fourier transform infrared spectrometer (FT-IR, TENSOR27, Bruker, Germany) and data collection program (OPUS, Optical User Software, Bruker, Germany) was used to investigate the effect of PPT on the degree of conversion (DC) of the 3DP denture resin specimens with microcapsules. Considering the PPT period, the infrared spectra of 3DP denture resin discs containing phytoncide-filled microcapsules, as well as those without microcapsules, were recorded between 4000 cm^{-1} and 400 cm^{-1} in the absorbance mode ($n=3$ per group), with a resolution of 1 cm^{-1} . The FTIR spectra of unpolymerized denture base resins were also recorded. DC of each 3DP denture resin specimen was calculated using the following equation.

$$\text{Degree of Conversion(DC)} = \left\{ 1 - \frac{Abs_{aliphatic}(\text{polymer})/Abs_{aromatic}(\text{polymer})}{Abs_{aliphatic}(\text{monomer})/Abs_{aromatic}(\text{monomer})} \right\} \times 100$$

where $Abs_{aliphatic}$ is the absorbance peak intensity of the aliphatic bond of the 3DP denture resin material measured from the peak at 1638 cm^{-1} and $Abs_{aromatic}$ is the absorbance peak intensity of the aromatic bond of the 3DP denture resin material measured from the peak at 1610 cm^{-1} .

To investigate the hardness of the 3DP denture resin disc, the discs with and without phytoncide microcapsules, subjected to different PPT protocols ($n=3$ per group), were prepared. Minimizing the effect of microcapsules on the surface topography, the testing surface of each disc was polished for clear examination of indentation using a polishing machine (Phoenix Beta, Bühler, Düsseldorf, Germany) at 150 rpm with 4000 grit SiC papers. The Vickers hardness test was performed on the polished surface of each disc using a diamond pyramid indenter (HM-220B, Mitutoyo, Japan) at 9.8 N load and repeated 10 times for each disc-shaped specimen.

The 3DP denture base-shaped specimens with and without microcapsules were subjected to different PPT protocols ($n=10$ per group), and their intaglio surfaces were digitized using a high-resolution laboratory scanner (Medit T710; Medit Corp, Seoul, Korea) in standard operation mode. The intaglio surface trueness of each specimen was evaluated using a 3D inspection software (Geomagic Control X; 3D Systems, Rock Hill, SC, USA) by superimposing the intaglio area of the reference CAD data of the denture base and the scanned intaglio surface data of the specimens. Three pairs of corresponding points were carefully selected on the tissue surface of each scanned denture base and reference CAD data to achieve preliminary alignment. Subsequently, the best-fit alignment with the iterative closest point-matching algorithm was performed. A color-coded 3D deviation map was displayed for each superimposition analysis of the 3DP specimens. The nominal deviation was set to $\pm 50\text{ }\mu\text{m}$, and the critical deviation was set to $\pm 500\text{ }\mu\text{m}$. The area within nominal deviation was displayed in green, while the area greater than nominal deviation was displayed in yellow (positive) or blue (negative). The surface deviation data measured in root-mean-square estimates (RMS, μm) were calculated using the formula below:

$$\text{RMS} = \frac{\sqrt{\sum_{i=1}^n (X_{1,i} - X_{2,i})^2}}{\sqrt{n}}$$

where $X_{1,i}$ is the point i on the reference data; $X_{2,i}$ is the point i on the test data; n is the total number of points.

The statistical analyses were conducted using the measured data of the 3DP denture resin specimens from five different treatment categories: (1) no microcapsule and 5-min PPT (negative control), (2) microcapsule and 5-min PPT (positive control), (3) microcapsule and 10-min PPT, (4) microcapsule and 20-min PPT, and (5) microcapsule and 30-min PPT. Based on the distribution of the collected data tested by the Shapiro–Wilk’s method and Levene’s test of equal variance, a non-parametric Kruskal–Wallis test and a post-hoc multiple comparison with Wilcoxon rank test adjusted by Bonferroni’s method were conducted for the data collected from the antifungal activity and degree of conversion analyses. For the measurements of each test for flexural strength (MPa), Vickers hardness (VH), and intaglio surface trueness (RMS, μm), one-way analysis of variance (ANOVA) and a post-hoc multiple comparison using Tukey’s method were performed for the differences among the groups. All statistical analyses were performed using IBM SPSS Statistics, v25.0; IBM Corp., Armonk, NY, USA), with a level of statistical significance (α) of 0.05.

Results

Based on the Kruskal–Wallis test, the numbers of fungal cell colonies (CFU/mL) on the discs with microencapsulated phytoncide were significantly different between the groups (Fig. 1, $P<0.001$). Adherence of fungal cell colonies to the disc surface was the lowest in the specimens with microcapsules and 10-min PPT, which indicates the highest antifungal activity. The specimens with microcapsules and 5-min PPT (positive control) showed significantly higher antifungal activity than those without microcapsules and 5-min PPT (negative control, $P<0.05$). However, as the PPT increases from 10 to 30 min, the numbers of fungal cell colonies attached to the discs filled with microcapsules significantly increased (all $P<0.05$).

Figure 2 shows the mean flexural strength values of the specimens subjected to different PPT protocols. The mean strength value of the specimens with no microcapsules and 5-min PPT (negative control) was $72.45 \pm 10.46\text{ MPa}$. With the same PPT, incorporating microcapsules into the denture base resin significantly decreased the mean value to $52.35 \pm 10.26\text{ MPa}$ (positive control, $P<0.05$). However, when subjected

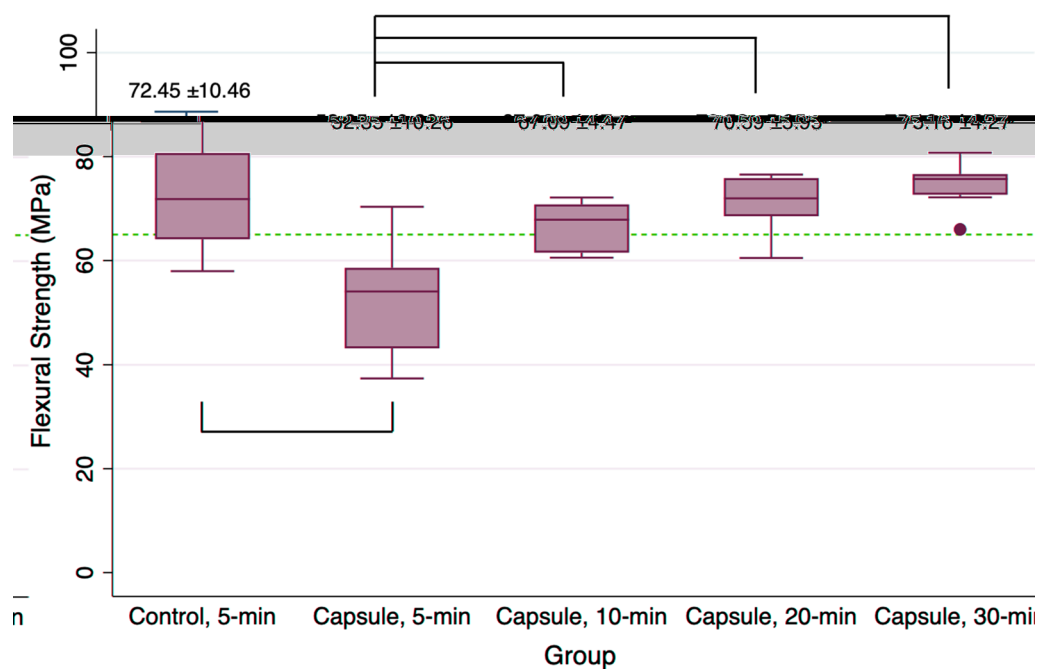


Fig. 2 Flexural strength values (MPa) of bar-shaped 3D-printed denture base resin specimens subjected to different post-polymerization time (PPT) protocols: 5-min, 10-min, 20-min, and 30-min. Control: 3D-printed denture base resin specimens without microcapsules; Capsule: 3D-printed denture base resin specimens with 5 wt% phytoncide-filled microcapsules. Significant differences between the groups are marked with black lines ($P < 0.05$). Flexural strength value of 65 MPa is marked in red dotted line

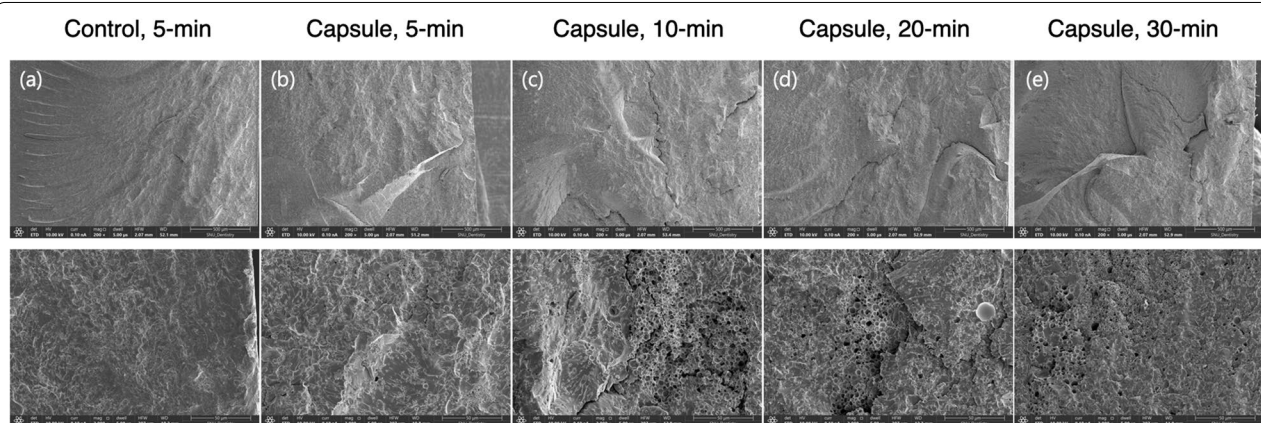


Fig. 3 Representative microscopic images (upper row, $\times 200$, and lower row, $\times 2000$) of fractured 3D-printed bar-shaped denture base specimens subjected to different post-polymerization time (PPT) protocols: 5-min, 10-min, 20-min, and 30-min. Control: 3D-printed denture base resin discs without microcapsules; Capsule: 3D-printed denture base resin discs with 5 wt% phytoncide-filled microcapsules. **a** Brittle fracture with smooth surface and chevron marks; **b–e** intermediate (ductile) fracture with rough surface and jagged areas. Note the microcapsules are evenly distributed over the fractured surfaces

to 10-min PPT, the mean strength value of the specimens with microcapsules significantly increased up to 67.09 ± 4.47 MPa ($P < 0.05$). As the PPT increased to 20 and 30 min, the specimens with microcapsules showed significantly improved mean strength values compared with those from the positive control group (all, $P < 0.05$).

The specimen with microcapsules and treated with 10-min PPT revealed comparable strength as those without microcapsules (negative control, $P > 0.05$). Microscopic observations (Fig. 3) revealed that the specimens from the negative control group showed brittle fracture patterns with flat, compact, and organized surfaces.

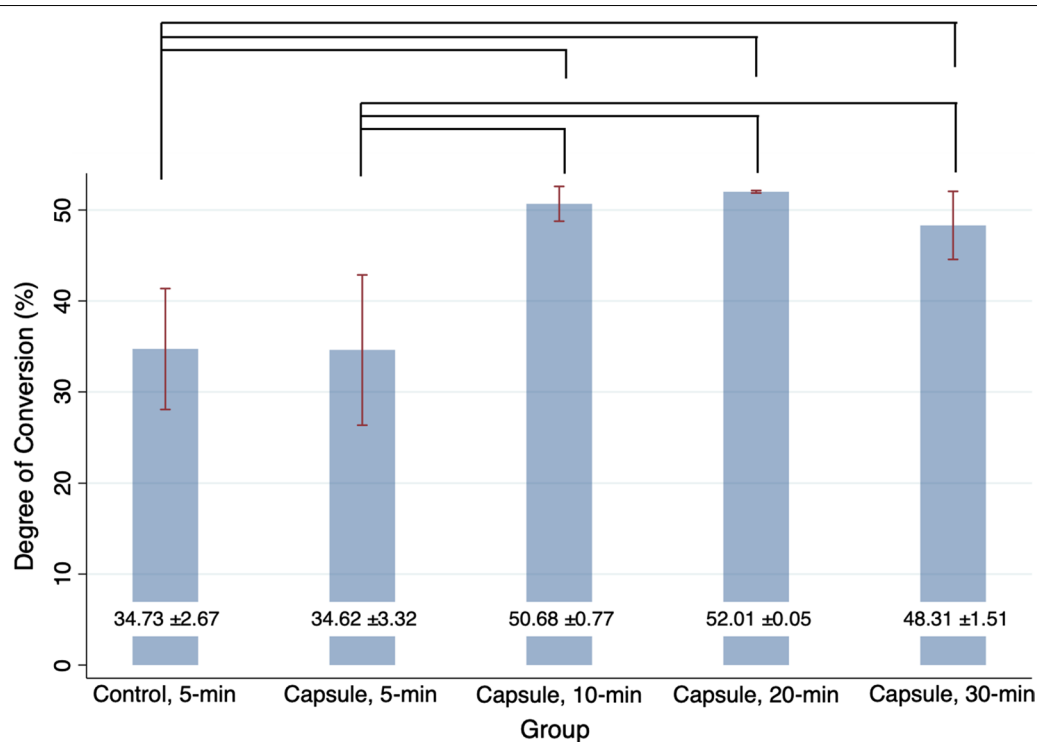


Fig. 4 Degree of conversion (%) of 3D-printed denture base resin discs subjected to different post-polymerization time (PPT) protocols: 5-min, 10-min, 20-min, and 30-min. Control: 3D-printed denture base resin discs without microcapsules; Capsule: 3D-printed denture base resin discs with 5 wt% phytoncide-filled microcapsules. Significant differences between the groups are marked with black lines ($P < 0.05$)

However, irrespective of the PPT protocols, all specimens with microcapsules showed typical patterns of intermediate fractures.

The DC values of the discs with microencapsulated phytoncide were significantly different between the groups, according to the Kruskal-Wallis analysis ($P = 0.014$). The 3DP denture resin discs filled with microcapsules and subjected to PPT for no less than 10 min showed significantly improved DC compared with those subjected to 5-min PPT ($P < 0.05$, Fig. 4). From the highest to lowest of the DC values, the discs subjected to 20-min PPT ($52.01 \pm 0.05\%$) were followed by those subjected to 10-min PPT ($50.68 \pm 0.77\%$), 30-min PPT ($48.31 \pm 1.51\%$), and 5-min PPT ($34.62 \pm 3.32\%$, positive control). No difference was found between the DC values of the specimens from the positive and negative control groups ($P > 0.05$). In addition, there was no statistical difference in the DC values between the specimens treated with 10-, 20-, and 30-min PPTs (all, $P > 0.05$).

The mean hardness value (HV) of the specimens without microcapsules and subjected to 5-min PPT (negative control) was significantly higher than that of those with microcapsules, regardless of the changes in PPT protocols (all, $P < 0.05$, Fig. 5). The mean hardness value of the specimens from the positive control group (18.06 ± 0.37)

was the lowest among the tested groups. However, on using PPT protocols of no less than 10 min, the mean hardness values of the specimens with microcapsules significantly increased compared with that of those subjected to 5-min PPT (all, $P < 0.05$). The mean hardness value was 18.99 ± 0.36 for the specimens subjected to 10-min PPT. No difference was detected between the groups filled with microcapsules and subjected to 10-min, 20-min, and 30-min PPT (all, $P > 0.05$).

The highest mean RMS value was $39.30 \pm 4.00 \mu\text{m}$ for the specimens with microcapsules and subjected to 5-min PPT. In contrast, the lowest value was $29.73 \pm 4.60 \mu\text{m}$ for those subjected to 20-min PPT. Under the same PPT of 5 min, the specimens with microcapsules showed significantly inferior trueness of the intaglio surface compared with that of those without microcapsules ($P < 0.05$, Fig. 6). As the PPT increased, all specimens with microcapsules and subjected to PPT for no less than 10 min showed better trueness than those subjected to 5-min PPT (positive control, $P < 0.05$). No statistical differences were detected between the specimens with microcapsules and subjected to 10-min, 20-min, and 30-min PPT protocols (all, $P > 0.05$). Furthermore, the specimens filled with microcapsules and treated with PPT

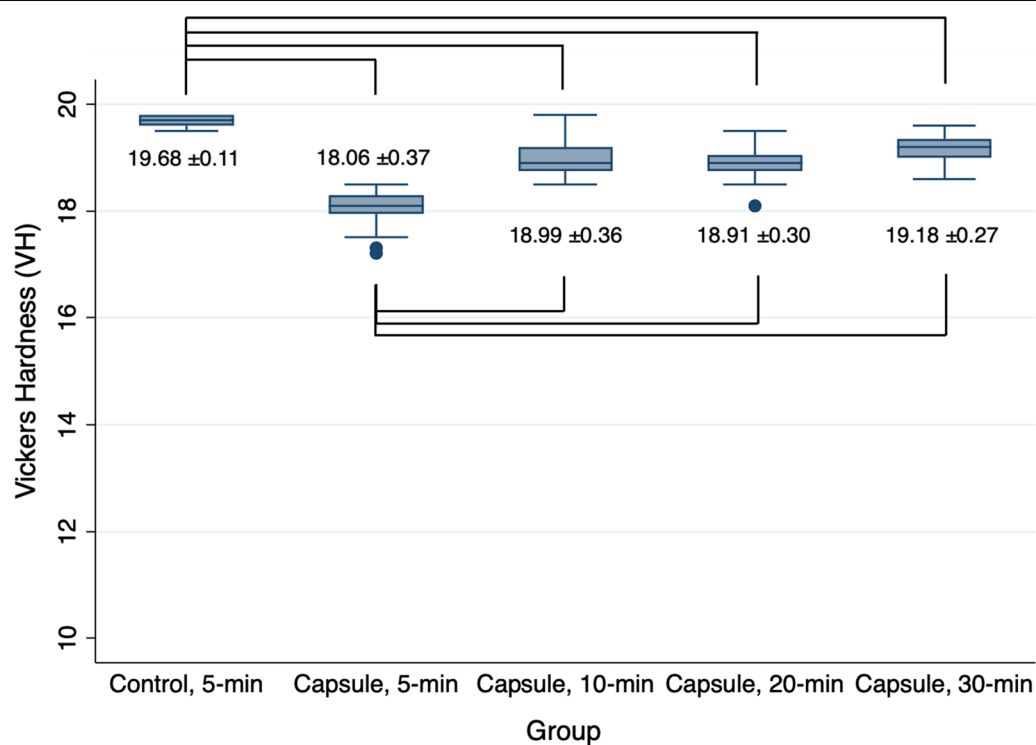


Fig. 5 Vickers hardness (VH) of 3D-printed denture base resin discs subjected to different post-polymerization time (PPT) protocols: 5-min, 10-min, 20-min, and 30-min. Control: 3D-printed denture base resin discs without microcapsules; Capsule: 3D-printed denture base resin discs with 5 wt% phytoncide-filled microcapsules. Significant differences between the groups are marked with black lines ($P < 0.05$)


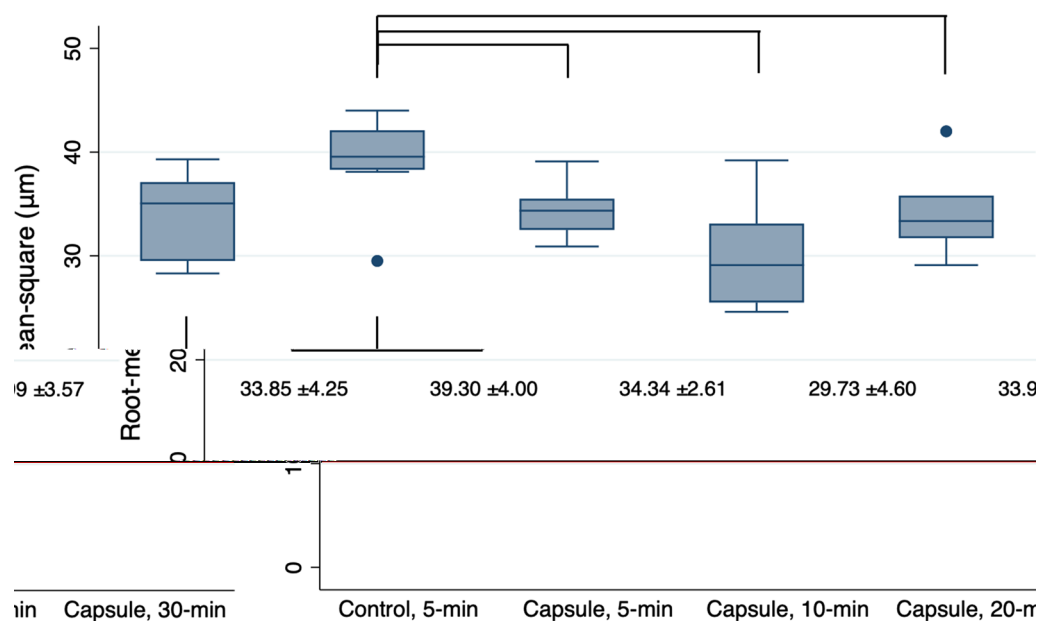


Fig. 6 Root-mean-square estimates of the 3D-printed denture base resin discs subjected to different post-polymerization time (PPT) protocols: 5-min, 10-min, 20-min, and 30-min. Control: 3D-printed denture base resin discs without microcapsules; Capsule: 3D-printed denture base resin discs with 5 wt% phytoncide-filled microcapsules. Significant differences between the groups are marked with black lines ($P < 0.05$)

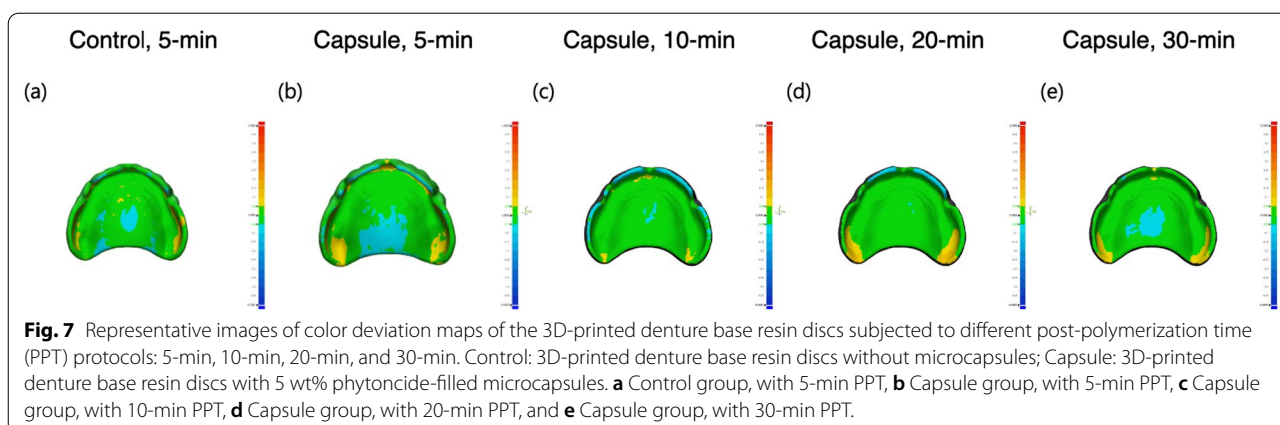

protocols for no less than 10 min were comparable with that of those without microcapsules (negative control, $P > 0.05$). However, regardless of the inclusion of microcapsules or the PPT protocol, all the specimens showed the RMS values under $50 \mu\text{m}$ for overall intaglio surfaces (Figs. 6 and 7). The color deviation map (Fig. 7) revealed that the specimens with microcapsules and subjected to 10-min PPT showed the most favorable pattern of surface deviation, with overall green area (within $50 \mu\text{m}$ of nominal deviation) with small regions of positive (yellow) or negative (blue) deviations.

Discussion

A group of researchers previously reported the fabrication of denture base material with antifungal activity against *C. albicans* using microencapsulation of phytoncide oil extract, mixing with a proper dispersant, and a digital light processing technique [31]. However, adding phytoncide-filled microcapsules may have affected the mechanical properties and dimensional accuracy of the 3DP denture base [37]. Although the flexural strength of the 3DP denture bases with microcapsules was comparable with that of bases without microcapsules, the degree of conversion, hardness, or dimensional accuracy was relatively decreased [31, 37]. To improve the flexural strength, degree of conversion, hardness, and intaglio surface trueness while maintaining the antifungal effect of the 3DP denture base, the current study focused on the effect of PPT, one of the most critical phases for 3D printing. Based on the findings of this study, the null hypotheses were rejected.

Flexural strength is essential for the success of denture treatment, as an external loading force is exerted on the dentures during mastication [43, 44]. The flexural strength of 3DP denture resin was enhanced by increasing the PPT [40]. In this study, compared with 5-min PPT, 3DP denture bases with phytoncide-filled

microcapsules showed improved flexural strength after increasing the PPT to 10 min. The measured strength was higher than 65 MPa, which is necessary for base polymers to be clinically acceptable based on the recommendations of the International Standard Organization [41]. This may be in accordance with the significantly increased DC in the specimens with microcapsules subjected to 10-min PPT compared with that of those subjected to 5-min PPT. Generally, the pores may act as the point of crack initiation during the fracture of PMMA resin; the microcapsules incorporated in the 3DP denture base resin may also function similarly [37]. In this study, the increased PPT was beneficial in enhancing the degree of conversion and, consequently, the flexural strength. Insufficient DC could reduce the mechanical properties of denture resins, where high DC is related to high conversion from monomers to polymers [45]. Furthermore, a denture base must have adequate hardness to resist surface wear during mastication or maintenance care, which may affect microbial accumulation when using complete dentures [46, 47]. The addition of microcapsules may have affected the Vickers hardness of 3DP denture base resin, still higher than the value reported in the literature [48]. In fact, by increasing PPT no less than 10 min, 3DP denture base resin with antifungal microcapsules showed sufficient Vickers hardness to withstand the clinical conditions [48].

For DLP-based workflow, a light source is essential as it supplies sufficient energy to induce polymerization of the photosensitive resin material, resulting in the formation of a highly cross-linked polymer [49]. Furthermore, a post-polymerization process is required to fully polymerize the object that has just been 3DP to finalize the desired mechanical and surface properties. Among the several parameters that could be modified, PPT is one of the easiest factors to approach. By changing the PPT, the accuracy, flexural strength, and hardness of the

3DP prosthesis have been improved, suggesting that the increase in PPT is advantageous [38–40]. In this study, by changing PPT from 5 min (positive control) to 10 min, the antifungal activity and mechanical properties of the 3DP denture base containing microcapsules were significantly improved. However, PPT protocols longer than 10 min did not increase the antifungal effect of the 3DP denture base. In addition, the intaglio surface trueness of the 3DP denture base with microcapsules, which is paramount for intimate tissue surface adaptation of the prosthesis, was also evaluated in this study. With the 10-min PPT protocol, the 3DP denture bases with microcapsules showed intaglio surface trueness comparable with that of those without.

The experimental design and calculated sample size evaluated in the present study were referred to previous in-vitro research by Jeon et al. and other recent in-vitro studies with similar research designs and test materials that reported significant differences [31, 37, 40]. However, the absence of a priori power analysis could be considered as a limitation of the this in-vitro research. In addition, further in-vitro research regarding physico-mechanical properties such as fracture toughness, compressive strength, and color stability of 3DP denture base with microcapsules is required. Since only one of the numerous 3D-printable denture base materials was tested in this study, further experiments with other denture materials are required.

Conclusion

Within the limitations of this in vitro study, the 3DP denture base containing phytoncide-filled microcapsules at 5 wt% concentration and subjected to 10-min PPT showed sufficient antifungal activity, while maintaining clinically comparable flexural strength, Vickers hardness, and intaglio surface trueness to the original 3DP denture base resin with no microcapsules. The antifungal activity and degree of conversion of 3DP denture base resin with microcapsules were significantly affected by the change of PPT. Further in-vitro and in-vivo studies are required before applying for clinical purpose.

Acknowledgements

Not applicable.

Author contributions

YHJ, WJL, and JHL carried out research and laboratory methodology. YHJ and HIY performed statistical analyses. YHJ and WJL wrote the draft. HIY edited the manuscript. HIY contributed to the study design, acquisition of the materials, interpretation of data, paper revision and supervised the research. All authors reviewed and approved the manuscript. All authors read and approved the final manuscript.

Funding

This research was supported by the Research Program to Solve Social Issues of the National Research Foundation of Korea (NRF) funded by the Ministry of

Science and ICT (NRF-2020R1F1A1075265), the Creative-Pioneering Researchers Program through Seoul National University (SNU), and grant no. 04-2021-0113 from the SNUDH Research Fund.

Availability of data and materials

The datasets generated and/or analyzed during the current study are available from the corresponding author upon reasonable request.

Declarations

Ethics approval and consent to participate

Not applicable.

Consent for publication

Not applicable.

Competing interests

The authors declare that they have no competing interests.

Author details

¹Dental Research Institute, Seoul National University School of Dentistry, Seoul, Republic of Korea. ²Department of Prosthodontics, School of Dentistry and Dental Research Institute, Seoul National University, 101, Daehak-ro, Jongno-gu, Seoul 03080, Republic of Korea.

Received: 29 July 2022 Accepted: 8 December 2022

Published online: 15 December 2022

References

- Saeed F, Muhammad N, Khan AS, Sharif F, Rahim A, Ahmad P, Irfan M. Prosthodontics dental materials: from conventional to unconventional. *Mater Sci Eng C Mater Biol Appl*. 2020;106:110167.
- Gundogdu M, Yanikoglu N, Bayindir F, Ciftci H. Effect of repair resin type and surface treatment on the repair strength of polyamide denture base resin. *Dent Mater J*. 2015;34:485–9.
- Alkurt M, Yeşil Duymuş Z, Gundogdu M. Effect of repair resin type and surface treatment on the repair strength of heat-polymerized denture base resin. *J Prosthet Dent*. 2014;111:71–8.
- Narva KK, Lassila LV, Vallittu PK. The static strength and modulus of fiber reinforced denture base polymer. *Dent Mater*. 2005;21:421–8.
- Darbar UR, Huggett R, Harrison A. Denture fracture-A survey. *Br Dent J*. 1994;176:342–5.
- Vallittu PK, Lassila VP, Lappalainen R. Evaluation of damage to removable dentures in two cities in Finland. *Acta odontol scand*. 1993;51:363–9.
- Kawara M, Komiya O, Kimoto S, Kobayashi N, Kobayashi K, Nemoto K. Distortion behavior of heat-activated acrylic denture-base resin in conventional and long, low-temperature processing methods. *J Dent Res*. 1998;77:1446–53.
- Nogueira SS, Ogle RE, Davis EL. Comparison of accuracy between compression- and injection-molded complete dentures. *J Prosthet Dent*. 1999;82:291–300.
- de Oliveira Limírio J, Gomes JML, Alves Rezende MCR, Lemos CAA, Rosa CDDR, Pellizzer EP. Mechanical properties of polymethyl methacrylate as a denture base: conventional versus CAD-CAM resin—A systematic review and meta-analysis of in vitro studies. *J Prosthet Dent*. 2021;21:S0022-3913.
- Javaid M, Haleem A. Current status and applications of additive manufacturing in dentistry: a literature-based review. *J Oral Biol Craniofac Res*. 2019;9:179–85.
- Yoon HI, Hwang HJ, Ohkubo C, Han JS, Park EJ. Evaluation of the trueness and tissue surface adaptation of CAD-CAM mandibular denture bases manufactured using digital light processing. *J Prosthet Dent*. 2018;120:919–26.
- Hwang HJ, Lee SJ, Park EJ, Yoon HI. Assessment of the trueness and tissue surface adaptation of CAD-CAM maxillary denture bases manufactured using digital light processing. *J Prosthet Dent*. 2019;121:110–7.
- Yoon SN, Oh KC, Lee SJ, Han JS, Yoon HI. Tissue surface adaptation of CAD-CAM maxillary and mandibular complete denture bases

- manufactured by digital light processing: a clinical study. *J Prosthet Dent*. 2020;124:682–9.
14. Jin MC, Yoon HI, Yeo IS, Kim SH, Han JS. The effect of build angle on the tissue surface adaptation of maxillary and mandibular complete denture bases manufactured by digital light processing. *J Prosthet Dent*. 2020;123:473–82.
 15. Da Silva WJ, Seneviratne J, Samaranayake LP, Del Bel Cury AA. Bioactivity and architecture of *Candida albicans* biofilms developed on poly (methyl methacrylate) resin surface. *J Biomed Mater Res B Appl Biomater*. 2010;94:149–56.
 16. He XY, Meurman JH, Kari K, Rautemaa R, Samaranayake LP. In vitro adhesion of *Candida* species to denture base materials. *Mycoses*. 2006;49:80–4.
 17. Samaranayake LP, MacFarlane TW. An in-vitro study of the adherence of *Candida albicans* to acrylic surfaces. *Arch Oral Biol*. 1980;25:603–9.
 18. Budtz-Jørgensen E. The role of *Candida albicans* in the development of stomatitis in denture wearers. *Med hyg (Geneve)*. 1975;33:1434–5.
 19. Arendorf TM, Walker DM. Denture stomatitis: a review. *J Oral Rehabil*. 1987;14:217–27.
 20. Cumming CG, Wight C, Blackwell CL, Wray D. Denture stomatitis in the elderly. *Oral Microbiol Immunol*. 1990;5:82–5.
 21. Gendreau L, Loewy ZG. Epidemiology and etiology of denture stomatitis. *J Prosthodont*. 2011;20:251–60.
 22. Webb BC, Thomas CJ, Willcox MD, Harty DW, Knox KW. *Candida*-associated denture stomatitis. Aetiology and management: a review. Part 3. Treatment of oral candidosis. *Aust Dent J*. 1998;43:244–9.
 23. Javed F, Samaranayake LP, Romanos GE. Treatment of oral fungal infections using antimicrobial photodynamic therapy: a systematic review of currently available evidence. *Photochem Photobiol Sci*. 2014;13:726–34.
 24. Emami E, Kabawat M, Rompre PH, Feine JS. Linking evidence to treatment for denture stomatitis: a meta-analysis of randomized controlled trials. *J Dent*. 2014;42:99–106.
 25. An S, Evans JL, Hamlet S, Love RM. Overview of incorporation of inorganic antimicrobial materials in denture base resin: a scoping review. *J Prosthet Dent*. 2021;27:S0022-3913.
 26. Chen SG, Yang J, Jia YG, Lu B, Ren L. TiO₂ and PEEK reinforced 3D printing PMMA composite resin for dental denture base applications. *Nanomaterials (Basel)*. 2019;9:1049.
 27. Monteiro DR, Gorup LF, Takamiya AS, de Camargo ER, Filho ACR, Barbosa DB. Silver distribution and release from an antimicrobial denture base resin containing silver colloidal nanoparticles. *J Prosthodont*. 2012;21:7–15.
 28. Totu EE, Nechifor AC, Nechifor G, Aboul-Enein HY, Cristache CM. Poly(methyl methacrylate) with TiO₂ nanoparticles inclusion for stereolithographic complete denture manufacturing—the future in dental care for elderly edentulous patients? *J Dent*. 2017;59:68–77.
 29. Silveira DQI, Lia EN, Massignan C, Stefani CM. Natural products for the treatment of denture stomatitis: a systematic review. *J Prosthet Dent*. 2021;8:S0022-3913.
 30. An S, Evans JL, Hamlet S, Love RM. Incorporation of antimicrobial agents in denture base resin: a systematic review. *J Prosthet Dent*. 2021;126:188–95.
 31. Jeon S, Jo YH, Yoon HI, Han JS. Antifungal effect, surface roughness, and cytotoxicity of three-dimensionally printed denture base with phytoncide-filled microcapsules: an in-vitro study. *J Dent*. 2022;120:104098.
 32. Salem MZM, El-Hefny M, Ali HM, Abdel-Megeed A, El-Settawy AAA, Böhm M, Mansour MMA, Salem AZM. Plants-derived bioactives: novel utilization as antimicrobial, antioxidant and phyto-reducing agents for the biosynthesis of metallic nanoparticles. *Microb Pathog*. 2021;158:105107.
 33. Abe T, Hisama M, Tanimoto S, Shibayama H, Mihara Y, Nomura M. Antioxidant effects and antimicrobial activities of phytoncide. *Biocontrol Sci*. 2008;13:23–7.
 34. Kang SK, Auh Q, Chun YH, Hong JP. Effect of *Chamaecyparis obtusa* tree phytoncide on *Candida albicans*. *J Oral Med Pain*. 2010;35:19–29.
 35. Lee MJ, Kim MJ, Oh SH, Kwon JS. Novel dental poly (methyl methacrylate) containing phytoncide for antifungal effect and inhibition of oral multi-species biofilm. *Materials*. 2020;13:371.
 36. An S, Judge R, Wong R, Arzmi M, Palamara J, Dashper S. Incorporation of the microencapsulated antimicrobial agent phytoncide into denture base resin. *Aust Dent J*. 2018;63:302–11.
 37. Jeon S, Jo YH, Yoon HI, Han JS. Effect of phytochemical-filled microcapsules with antifungal activity on material properties and dimensional accuracy of denture base resin for three-dimensional printing. *BMC Oral Health*. 2022;22:178.
 38. Lee BI, You SG, You SM, Kim DY, Kim JH. Evaluating the accuracy (true-ness and precision) of interim crowns manufactured using digital light processing according to post-curing time: an in vitro study. *J Adv Prosthodont*. 2021;13:89–99.
 39. Kim D, Shim JS, Lee D, Shin SH, Nam NE, Park KH, Shim JS, Kim JE. Effects of post-curing time on the mechanical and color properties of three-dimensional printed crown and bridge materials. *Polymers*. 2020;12:2762.
 40. Aati S, Akram Z, Shrestha B, Patel J, Shih B, Shearston K, Ngo H, Fawzy A. Effect of post-curing light exposure time on the physico-mechanical properties and cytotoxicity of 3D-printed denture base material. *Dent Mater*. 2022;38:57–67.
 41. International Organization for Standardization. ISO 20795-1: 2013. Dentistry - Base polymers - Part 1: Denture base polymers. 2nd ed.
 42. Monsen T, Lövgren E, Widerström M, Wallinder L. In vitro effect of ultrasound on bacteria and suggested protocol for sonication and diagnosis of prosthetic infections. *J Clin Microbiol*. 2009;47:2496–501.
 43. Murakami N, Wakabayashi N, Matsushima R, Kishida A, Igarashi Y. Effect of high-pressure polymerization on mechanical properties of PMMA denture base resin. *J Mech Behav Biomed Mater*. 2013;20:98–104.
 44. Kawaguchi T, Lassila LV, Sasaki H, Takahashi Y, Vallittu PK. Effect of heat treatment of polymethyl methacrylate powder on mechanical properties of denture base resin. *J Mech Behav Biomed Mater*. 2014;39:73–8.
 45. Franz A, König F, Lucas T, Watts DC, Schedle A. Cytotoxic effects of dental bonding substances as a function of degree of conversion. *Dent Mater*. 2009;25:232–9.
 46. Cevik P, Yildirim-Bicer AZ. The effect of silica and prepolymer nanoparticles on the mechanical properties of denture base acrylic resin. *J Prosthodont*. 2018;27:763–70.
 47. Machado AL, Breeding LC, Vergani CE, da Cruz Perez LE. Hardness and surface roughness of reline and denture base acrylic resins after repeated disinfection procedures. *J Prosthet Dent*. 2009;102:115–22.
 48. Al-Dwairi ZN, Al Haj Ebrahim AA, Baba NZ. A comparison of the surface and mechanical properties of 3D printable denture-base resin material and conventional polymethylmethacrylate (PMMA). *J Prosthodont*. 2022. Epub ahead of print.
 49. Zakeri S, Vippola M, Levänen E. A comprehensive review of the photopolymerization of ceramic resins used in stereolithography. *Addit Manuf*. 2020;35:101177.

Publisher's Note

Springer Nature remains neutral with regard to jurisdictional claims in published maps and institutional affiliations.

Ready to submit your research? Choose BMC and benefit from:

- fast, convenient online submission
- thorough peer review by experienced researchers in your field
- rapid publication on acceptance
- support for research data, including large and complex data types
- gold Open Access which fosters wider collaboration and increased citations
- maximum visibility for your research: over 100M website views per year

At BMC, research is always in progress.

Learn more biomedcentral.com/submissions

